

Size-exclusive Nanosensor for Quantitative Analysis of Fullerene C₆₀: A Concept Paper

SAMUEL N. KIKANDI, VERONICA A. OKELLO, QIONG WANG, *¹OMOWUNMI A. SADIK

Center for Advanced Sensors & Environmental System (CASE)

Department of Chemistry

State University of New York-Binghamton

P.O. Box 6000

Binghamton, NY 13902-6000

KATRINA. E.VARNER

US-EPA/NERL

Environmental Sciences Division

P.O. Box 93478-3478

Las Vegas, NV 89193-3478

SARAH A. BURNS

Department of Chemistry

359 Natural Sciences Complex

State University of New York-Buffalo

Buffalo, NY 14260-3000

*Corresponding Author:(607)777-4132;Fax:(607)777-4132,E-mail:osadik@binghamton.edu

ABSTRACT

This paper presents the first development of a mass-sensitive nanosensor for the isolation and quantitative analyses of engineered fullerene (C_{60}) nanoparticles, while excluding mixtures of structurally similar fullerenes. Amino-modified beta cyclodextrin (β -CD-NH₂) was synthesized and confirmed by ¹HNMR as the host molecule to isolate the desired fullerene C_{60} . This was subsequently assembled onto the surfaces of gold-coated quartz crystal microbalance (QCM) electrodes using N-Dicyclohexylcarbodiimide/N-hydroxysuccinimide (DCC/NHS) surface immobilization chemistry to create a selective molecular configuration described as (Au)-S-(CH₂)₂-CONH-*beta*-CD sensor. The mass change on the sensor configuration on the QCM was monitored for selective quantitative analysis of fullerene C_{60} from a C_{60}/C_{70} mixture and soil samples. About $\sim 10^{14}$ - 10^{16} C_{60} particles/cm² were successfully quantified by QCM measurements. Continuous spike of 200 μ l of 0.14 mg C_{60} /ml produced changes in frequency ($-\Delta f$) that varied exponentially with concentration. FESEM and Time-of-Flight Secondary Ion Mass Spectrometry (ToF-SIMS) confirmed the validity of sensor surface chemistry before and after exposure to fullerene C_{60} . **The utility of this sensor for spiked real-world soil samples has been demonstrated. Comparable sensitivity was obtained using both the soil and purified toluene samples. This work demonstrates that the sensor has potential application in complex environmental matrices.**

KEYWORDS: Fullerenes, Nanotechnology, Engineered Nanomaterials, Implications, Toxicity, Cyclodextrin, Nanosensors.

Introduction:

The discovery of fullerenes in 1985 has ushered in an explosive growth in the applications of engineered nanomaterials (ENMs) and products (1-5). The rapid development of nanotechnology and the increasing production of nanomaterials-based products and processes present great opportunities and challenges. To date, the potential impacts of nanomaterials on human health and the environment have been limited due to insufficient understanding of the risks associated with its development, manipulation and wide-ranging applications. The first step in assessing the risks posed by ENMs is to develop a broad array of analytical tools and methods that are applicable to a wide range of manufactured nanomaterials. Conventional methods of assessing the properties and characteristics of raw nanomaterials focus on the size distribution and effects. They are, however, unsuitable for detection and quantification of complex environmental samples or for differentiating between the total or dissolved metal fractions or metal oxidation states. The toxicity, detection and characterization of nanomaterials are dependent on factors such as functionalization, geometry, and the type of nanomaterials. For example, the cytotoxicity of fullerenes can be decreased following its hydroxylation with 24 hydroxyl groups(3), while the cytotoxicity of carbon nanomaterials may be enhanced if it was functionalized with carboxylic acid moieties(4). The potential toxicity of fullerenes and its derivatives is still a subject of intense discussion (5). Some reports depict fullerenes as non-toxic while others demonstrate their ability to both quench and generate reactive oxygen species(ROS) (6), which may lead to DNA damage(7). Additionally, positive cytotoxicity and genotoxicity have been reported for the water-soluble C_{60} aggregates (nC_{60}) despite its low hydrophobicity(8).

The first step to a better understanding of the fate and transport of fullerenes and other nanomaterials is to develop reliable metrology and analytical sensors. These offer novel screening and monitoring approaches towards a better understanding of engineered nanomaterials. Nanosensors can be classified under two main categories(1, 9): (i) Nanotechnology-enabled sensors or sensors that are themselves nanoscale or have nanoscale materials or components, and (ii) Nanoproperty-quantifiable sensors. Nanomaterials dimensions are on the same scale as biomolecules, which unveils exciting possibilities for their interaction with biological species, such as microbial, tissue, cells, antibodies, DNA and other proteins. Type I sensors have been used for the construction of enzyme sensors, immunosensors and genosensors, to achieve direct wiring of enzymes and relative components to electrode surface, to promote spectroelectrochemical reaction, to impose barcode for biomaterials and to amplify signal of biorecognition event[(10, 11). Extensive research papers and reviews using nanomaterials for chemical and bioassays have since been published (1, 5).

Despite the enormous literatures, there are few sensors to measure nanoscale properties or sensors belonging to Type II. This class of nanosensors is an area of critical interest to nanotoxicology, detection and risk assessment, as well as for monitoring of environmental and/or biological exposures to nanomaterials such as fullerene C₆₀. This is important because engineered fullerenes C₆₀ which are prepared *via* thermal reactions always exist as a mixture of C₆₀, C₇₀ and higher homologues. While supramolecular complexation with host-guest recognition is a well-studied topic (12-14), and nanomaterials have been widely reported as components of sensing or other applications, to the best of our knowledge, there has neither been fullerene sensors reported nor the assembly of β -CD achieved onto mass selective transducers for C₆₀ nanoparticle sensing applications. This paper presents the development of Category II nanosensor for the isolation and quantitative analyses of engineered fullerene C₆₀ while excluding other structurally similar fullerenes C₇₀ and higher homologues.

Experimental section:

Microgravimetric measurements: Microgravimetric measurements were performed following a conventional procedure(15). Briefly, all microgravimetric QCM experiments were performed using a QCA 917-quartz crystal analyzer (Seiko EG&G). This was an open circuit system where only the gold-coated quartz crystal (QA-A9M-Au(M)) from Advanced Meas. Tech. (Oak Ridge, TN)working electrode (QCM, area $\sim 0.2 \text{ cm}^2$) was connected in the absence of the auxiliary and the reference electrodes.). The resonators consisted of gold thickness layer of 300 nm and a frequency resolution of 0.1 Hz at a sampling rate of 100 ms, allowing excellent sensitivity down into the nanogram region. These resonators were mounted onto a Teflon well-type electrochemical cell(15) then soaked with test solutions. Buffalo River Sediments soil samples were obtained from, National Institute of Standards and Technology, Gaithersburg, MD 20899, (Lot # 8704).

Synthesis of Cyclodextrin Derivatives: The sensor fabrication started with the synthesis of β or γ -cyclodextrin derivatives consisting of amino-functionalized derivatives of cyclodextrins designated as: β -CD-NH₂ **1** and γ -CD-NH₂ **2**(**Supplementary Figure 1A**). The synthesis of these derivatives utilized previous literature procedures with slight modifications (16): Briefly, 0.72 g of either β -CD or γ -CD was treated with 1.2 g toluene-2-sulfonyl chloride, TsCl (Sigma-

Aldrich,US) and ethylenediamine(1 ml)(Sigma-Aldrich, US) in 20 mL pyridine (Sigma-Aldrich, US) and the mixture was refluxed for 7 hours resulting in yellow solids. The yellow solids were designated as β -CD-NH₂ **1** or γ -CD-NH₂ **2**. These synthetic products (**1** & **2**) were stored under ultra high purity nitrogen (UHP) until they were utilized for the immobilization onto the QCM surface.

Successful synthesis of **1** and **2** were confirmed by ¹HNMR spectra recorded on a Bruker AM 360 spectroscopic system equipped with 8.45 T magnet and multinuclear and inverse detection capabilities at 360MHz at 20 °C using D₂O solvent (**Supplementary Figure 1B**). The ¹HNMR sample concentrations were approximated as 25 mg/mL of β -CD, β -CD-NH₂ **1**, γ -CD and γ -CD-NH₂ **2**. Compound **1**, showed characteristic NH₂ and methylene protons with chemical shifts at δ ~2.2ppm and δ ~3.0 ppm respectively. Compound **2** showed similar chemical shifts at δ ~ 2.2 and 2.8 ppm for NH₂ and methylene protons respectively (data not included). Chemical shifts from both compounds **1** and **2** were consistent with the calculated theoretical chemical shifts values using ChemDraw for NH₂ and CH₂-protons (δ =2.0 and δ =2.8 ppm respectively). These results were consistent with literature precedence (12, 16, 17). In addition, this modification is not only important for the immobilization chemistry but also for the enhanced cyclodextrin guest-host activity. For example, the depth of the cavity is extended from 0.78 nm to 1.10 nm and the hydrophilic nature of both ends of the β -CD cavity is changed due to the methyl groups attached to the O-2, O-3, or O-6 of the cyclodextrin(18). Current work does not include studies on the effect of the cyclodextrin modification or did not eliminate the role of such chemistry in the sensor fabrication.

Cyclodextrin Assembly onto the QCM Transducer: Compounds **1** and **2** were immobilized separately on QCM via the DCC/NHS chemistry (Sigma-Aldrich) (15). First, QCM was cleaned in Piranha solution (H₂SO₄: H₂O₂=3:1, v/v) to remove any organic impurities and rinsed in copious amount of ethanol/water (1:1, v/v) mixture and dried gently in a stream of nitrogen. The cleaned QCM was subjected to the procedure shown in **Supplementary Figure 1C**. Briefly, the QCM was soaked for 1 hour in 1 mM 3, 3' dithiopropionic acid, DTPA (Sigma-Aldrich) in acetone to facilitate the formation of the sensor molecular configuration hereby designated as QCM (Au)-S-(CH₂)₂-COOH acid **3**. The QCM with immobilized acid was rinsed again to remove any unreacted DTPA and then soaked in a mixture of 400 μ L of 5mM DCC (in acetone) plus 400 μ L of ~ 5.0 mg/ml (in water) either β -CD-NH₂ **1** or γ -CD-NH₂ **2**. About 400 μ L of 2 mM NHS (in acetone) was added and the conjugation reaction allowed for 30-60 minutes. During this conjugation process, carbodiimide molecule reacts with the carboxyl groups on the already immobilized DTPA molecule (*via* Au-S bond). This gives a highly reactive *O*-acylurea, which then reacts with the nucleophilic amines in **1** or **2** to form a stable amide(19). NHS is added to stabilize the unstable carbodiimides (19). The sensor was then rinsed to remove any excess reagents and dried gently in a stream of nitrogen. This modified QCM assembly was designated as QCM-S-(CH₂)₂-CONH- β -CD sensor, **4**.

Isolation & Quantitation of Fullerene C₆₀: Several methods have been reported for separation of C₆₀ especially in complex mixtures consisting of fullerene C₇₀ and higher homologues (5, 20, 21). Complexation of *beta*-cyclodextrin and fullerene C₆₀ (β -CD-C₆₀) is known to be a tight fit compared to that of γ -CD-C₆₀ (18). The affinity is dictated by the CD cavity polarity and sizes as well as the stability constants. In aqueous solution the stability of

the β -CD: C_{60} = 2: 1 complex is $k=1.696 \times 10^5 \text{ dm}^6 \text{ mol}^{-2}$) while that of γ -CD- C_{60} is $k=2.66 \times 10^7 \text{ dm}^6 \text{ mol}^{-2}$. This is a dynamic equilibrium that implies that C_{60} spends more time in β -CD cavity than that of γ -CD, an important consideration for the proposed nanosensor. The binding abilities and solubility for both C_{60} and C_{70} are higher in toluene solution (22). Isolation and quantitation was achieved on a mass-sensitive QCM-S-(CH₂)₂-CONH- β -CD nanosensor, **4**. In solution, the complexation of C_{60} : β -CD=1: 2 are favored (76 %), 1: 1(61 %) and 2:1(44 %) (16). β -CD interaction with fullerenes is also selective because it complexes with C_{60} (19) and not with C_{70} or higher analogues(16, 23). This is because C_{60} (diameter $\approx 0.7 \text{ nm}$) is smaller than the internal diameter of β -CD cavity (diameter $\approx 0.79 \text{ nm}$) while that of C_{70} is larger (diameter $\approx 0.8 \text{ nm}$). While C_{60} is spherical, C_{70} is ovoid in shape which makes its recognition by β -CD more difficult (**Scheme 1 Supplementary Information**). Therefore, when β -CD modified QCM sensor is exposed the mixture, C_{60} fits into the hydrophobic cavity while C_{70} is excluded on the basis of their size and shape. The sensor design was restricted to the isolation of C_{60} from this type of mixture because of its potential industrial practical utility and future improvement for environmental monitoring.

Nanosensor measurements: The QCM (Au)A-S-(CH₂)₂-CONH- β -CD sensor, **4** was mounted to QCA 917-quartz crystal analyzer which was connected to EG&G PAR 263A potentiostat for data acquisition. In triplicates, exactly 200 μL of 0.14 mg/mL of C_{60} or C_{70} in toluene and control (toluene only) were placed on the modified QCM separately and the change in frequency was monitored over time. The changes were recorded as the immobilized β -CD on the QCM capturing the guest hydrophobic fullerene particles into their hydrophobic cavities(12). These events (16) caused the resonant frequency to decrease in proportion to the mass according to Saurbrey equation

$$\Delta f = -\left(\frac{2fo^2}{s\sqrt{\mu\rho}} \right) \Delta m \text{ (24); where } \Delta f \text{ is the change in crystal frequency (which is the measured parameter), } fo \text{ is the fundamental resonant frequency of the crystal (in the electrolyte), } s \text{ is the electrode area (} \sim 0.2 \text{ cm}^2 \text{), } \mu \text{ is the shear modulus of the crystal (} = 2.947 \times 10^{11} \text{ g cm}^{-1} \text{ s}^{-2} \text{), } \rho \text{ is the density of the quartz (} = 2.648 \text{ g cm}^{-3} \text{) and } \Delta m \text{ is the change in mass at the surface of the crystal resonator. Using this equation, frequency changes can be converted to adsorbed mass and finally converted to the number of captured } C_{60} \text{ fullerene particles (24).}$$

Sensor surface characterization using ToF-SIMS & FESEM: Time of Flight-Secondary Ion mass spectrometry (ToF-SIMS) and Field Emission Scanning Electron Microscope (FESEM), Zeiss Supra™ 55VP were used to characterize the surface chemistry during fabrication and testing experiments. Relevant details on the description of FESEM and ToF-SIMS are available in the supporting information: sensor surface characterization.

Results and Discussion

Selective Fullerene C_{60} Quantitation using the Mass Sensor: As noted earlier, β -CD modified QCM sensor **4** was exposed to various concentrations of C_{60} or C_{70} in toluene. QCM relationship between the resonance oscillation frequency of piezoelectric crystal and interfacial mass change was monitored according to the Saurbrey equation (24). A decrease in frequency of 1Hz corresponds to 1.34 ng (25) and this was used to calculate the mass of the

captured fullerenes. In this work, the sensor results are shown in **Figure 1** when the sensor was exposed to 0.14 mg /ml of C₆₀, C₇₀ and the control. Clearly, the sensor exposed to C₆₀ showed significant decrease in frequency over time while C₇₀ and the control (toluene) remained relatively steady indicating that no significant mass was adsorbed on the QCM. This observation was consistent with the predicted sensor performance and it proved that it is indeed feasible and selective. The selective capture of C₆₀ was not only feasible but was also found to be consistent with the expected β -CD-C₆₀ guest-host interactions (12, 16). This is evident from the results. For example in **Figure 1**, the change in frequency was recorded as $\sim 10618\text{Hz}$ (or $\sim 14228\text{ng}$), which corresponds to $\sim 5.95 \times 10^{16}$ C₆₀ particles/cm². Using a 1:10 dilution, the observed Δf was $\sim 1098.3\text{ Hz}$ ($\sim 1471.72\text{ ng}$) or 6.15×10^{15} C₆₀ particles/cm² and with a 1:100 dilution, the Δf was $\sim 90.4\text{Hz}$, or 3.77×10^{14} C₆₀ particles /cm². Overall, about $\sim 10^{14}$ - 10^{16} C₆₀ particles/cm² range was consistently quantified by this sensor from 0.14 mg C₆₀ /ml solution at 1:1, 1:10 and 1:100 dilutions.

Assuming that a perfect β -CD (diameter= 0.78 nm) assembled on an active sensing electrode surface area of 0.2 cm², $\sim 1.90 \times 10^{14}$ β -CD /cm² should fit on the QCM sensor. If single C₆₀ were isolated, $\sim 10^{14}$ C₆₀/cm² would be obtained from the observed results. However, the measured values were higher ($\sim 10^{14}$ - 10^{16} C₆₀/cm²) suggesting that both single nC₆₀ and clusters, (C₆₀)_n had been captured since these exist as fractal system in toluene (26). Also cyclodextrins are likely to co-adsorb the fullerenes and solvent molecules or other trace impurities during the process. This co-adsorption probably explains why the number frequency changes and measured particles were larger than anticipated. The discrepancy here was considered insignificant since the controls remained steady during measurements as evident from **Figures 1, 2 and 3**. Similar variations were noted for DTPA during the sensor fabrication. The approximate number of DTPA and β -CD molecules calculated during the immobilization step was $\sim 3.3 \times 10^{15}$ / cm² and $\sim 5.9 \times 10^{14}$ / cm² respectively. The experimental number of β -CDs ($\sim 10^{14}$) and that of the predicted support molecules β -CD ($\sim 10^{14}$) were within the same order of magnitude. However, that of DTPA was 10-fold higher than β -CD, an indication that excess DTPA did not react with β -CD during the fabrication steps.

The quantitation of fullerene C₆₀ nanoparticle was found to be consistent with other immobilized host-guest chemistry on similar QCM surface area. For example, Stobiecka and co-workers reported $\sim 10^{12}$ - 10^{13} molecules/cm² of oligonucleotides immobilized on QCM(25). It is obvious that the density of the immobilized molecules or particles on the electrode is expected to vary with their respective molecular sizes hence the slight variation observed. Additionally, this study also agrees with other works involving β -CD inclusion chemistries (27).

Sensor Dose-dependent Response: Dose-dependent responses were subsequently tested using a conventional procedure (15, 28). A freshly fabricated QCM sensor modified with β -CD **4** was immersed into an electrochemical cell containing 6 ml toluene and a stirring magnet. The cell was connected to quartz analyzer. The program and a timer were started simultaneously. Exactly, 200 μL of 0.15 mg C₆₀/ml or blank (toluene) were spiked separately at selected matching time intervals (100 s). **Figure 2** shows the results obtained. Spiking of C₆₀ solutions showed characteristic stair-case like profile along with decreasing frequency while the control remained steady (**Figure 2 (A)**). The change in frequency ($-\Delta f$) varied exponentially with mass change (Δm) with $R^2 = 0.998$ (**Figure 2 (B)**).

Fullerene C₆₀ & C₇₀ Interaction with γ -CD: In the previous section, it was demonstrated that β -CD (diameter=0.78 nm) could selectively capture fullerene C₆₀ (diameter = 0.7nm) and

not C₇₀ (diameter = 0.8 nm) from toluene solution. Hypothetically, unlike β -CD, the use of γ -CD is expected to capture both C₆₀ or C₇₀ with no effect on the control. This is because of its larger cavity (diameter = 0.95 nm) compared to that of either the C₆₀ or C₇₀. This hypothesis was tested by preparing the QCM sensor with γ -CD assembly in place of β -CD using the same procedure described earlier. The results obtained for C₇₀ and C₆₀ are shown in **Figures 2(A) and (B)** respectively under **Supplementary Information**. As predicted, C₆₀ and C₇₀ were detected while the controls remained steady.

This is also consistent with the consideration that γ -CD cavity diameter is larger than the diameter C₆₀ or C₇₀. γ -CD+C₇₀ showed an ideal change in frequency where the decrease reaches a plateau as no more active binding sites (cavities) were available for C₇₀. It was predicted that a perfect γ -CD (diameter, $d=0.95\text{nm}$) has cavity surface area of about $\sim 7.1 \times 10^{-15} \text{ cm}^2$ each. Since the QCM area was approximated as 0.2 cm^2 then it is expected that up to $\sim 2.8 \times 10^{13} \text{ } \gamma\text{-CD particles/cm}^2$ would fit on the QCM sensor. Experimental results (**Figure 2A Supplementary Information**) showed that in the presence of C₇₀ a $\Delta F \sim -1836551\text{Hz}$ was obtained, which corresponds to $\sim 9.00 \times 10^{18} \text{ C}_{70} \text{ particles/cm}^2$ captured. For C₆₀, ΔF was recorded as $\sim -1242450 \text{ Hz}$, which corresponds to $\sim 7.1 \times 10^{18} \text{ C}_{60} \text{ particles/cm}^2$. Obviously, these numbers of particles were higher than anticipated. This is consistent with earlier results of C₆₀ detection by β -CD sensor, an indication that both single and clustered or aggregated fullerenes were detected (26). For a 1:20 concentration ratio of C₆₀/C₇₀ mixture no interference was observed, however when the concentration of C₇₀ was increased to 50 fold a lower number of C₆₀ were captured on the sensor (**Figure 2 C supplementary information**)

Sensor Surface characterization using ToF-SIMS & FESEM: ToF-SIMS was used to determine if the fragmentation ions and spatial distribution of the attached molecules was actually achieved as predicted. This utilized low primary ion dosages (so called static SIMS) to identify the molecular and fragment ions related to the gold substrate, DTPA, β -CD and the C₆₀ Components. The liquid metal ion source (Bi_n^{q+}) was used since this ion source can analyze a surface with high spatial resolution (to 50 nm) and with high sensitivity for molecular ion species (29). The characteristic fragment ions identified in the static analysis were then used to construct the chemical images to identify the spatial distribution of these components. ToF-SIMS chemical imaging was initially used to determine if the chemical components of S-(CH₂)₂-CONH- β -CD were present at the surface of the gold substrate. This was achieved by analyzing the gold substrate before and after the functionalization chemistry. Once it was determined that the DTPA was present, a sample containing the acid component with the β -CD attached was analyzed to determine if both of these components were present and had similar spatial distribution. During this study it was observed that the acid and β -CD components formed surface domains in a similar spatial relation to the gold substrate and that these domains were also located in the same spatial arrangement as C₆₀.

This observation was followed by the identification of the characteristic fragment ions associated with the three major components of the sensor configuration: the gold substrate, the cyclodextrin, and fullerene (C₆₀). The gold ions formed a well characterized pattern in ToF-SIMS analysis which can be observed in a mass spectrum as clusters of gold (Au_n). The identified fragment ions associated with gold substrate were $\text{Au}^+(m/z 197)$ and $\text{Au}_3^+(m/z 591)$ while those associated with DTPA included $\text{C}_2\text{H}_4\text{S}^-(m/z 60)$; $\text{C}_3\text{H}_5\text{SO}_2^-(m/z 105)$; $\text{C}_6\text{H}_9\text{S}_2\text{O}_4^-(m/z 209)$ and $\text{C}_{12}\text{H}_{19}\text{S}_4\text{O}_8^-(m/z 419)$ as shown in **Supplementary Table 1 & Supplementary Figure 3**. The fragment loss of cyclodextrin has been described by Rabara and co-workers

who utilized ToF-SIMS for the analysis of β -cyclodextrin and identified a series of fragment ions ($C_8H_{13}O_7^-$, $C_{14}H_{23}O_{12}^-$, $C_{20}H_{33}O_{17}^-...$) in the negative ion acquisition mode(30). This fragmentation was observed in the formulated QCM and a mass spectrum of a representative cyclodextrin peak can be found in supporting information (**Supplementary Table 2 & Supplementary Figure 4**). The fragment loss of C_{60} has previously been described as being a C_2 loss (C_{58} , C_{56} , $C_{54}...$) from the C_{60} initial mass(31, 32). This fragmentation loss pattern was not observed in the fullerene soaked QCM; only the peak for C_{60}^- at m/z 720 was observed (**Figure 3**). Other fragments associated with C_{60} included m/z 721, 722, 723 and 724 which is representative of the isotopic pattern of C_{60} . This was a critical step and the results confirmed that C_{60} had been captured from toluene by the sensor. In toluene, C_{60} is known to exist as a fractal system consisting of both single (C_{60}) and aggregates/clusters, $(C_{60})_n$ (26). Therefore, either single C_{60} , cluster $(C_{60})_n$ or both were isolated and measured by the sensor. While it is obvious for the detection of the single C_{60} particles by the predicted β -CD - C_{60} complexation, it is not so for the aggregated fullerenes, $(C_{60})_n$. In this work, ToF-SIMS results showed evidence of single fullerene particles (m/z 720) and the isotopic fragments. Detection of higher clusters of C_{60} proved to be difficult by ToF-SIMS due to the roughened surface which lowered the useable mass range of the sensors as observed. This however does not eliminate the possibility that C_{60} clusters exist at the surface.

FESEM (Zeiss SupraTM 55VP) was further used to provide evidence of such clusters on the sensor as long as they are at least within 1.7 nm - 4 nm range (33). Fullerene clustering process is not clearly understood but available literature point to a radical mechanism since it is suppressed by addition of radical scavengers (34). Formation of stable fullerene $(C_{60})_n$ clusters with sizes >1.2 nm in toluene solution and aggregation number $n \geq 3$ is known(26). The number (n) is usually within $3 \leq n \leq 60$ with the spherical $(C_{60})_{55}$ cluster (4.6 nm) being the most stable(26). Using the FESEM, the sensor was characterized and results showed presence of near spherical clusters ≥ 200 nm (**Supplementary Figure 5**) suggesting a few hundreds of C_{60} particles per cluster. Overall, ToF-SIMS and FESEM confirmed the presence of both single and clustered C_{60} on the sensor consistent with the fractal system literature (26).

Spatial Distribution: Chemical imaging of the ToF-SIMS data were used to determine the spatial distribution of the major components on the QCM during each phase of formulation. The images were analyzed using the Ion Image Software program and Image J, a public domain Java-based image processing program. The combination of these programs was used to study the fragments' spatial distributions(35). The first sample analyzed contained the gold substrate treated with DTPA only. The chemical images indicated that the acid was present on the QCM surface with distinct segregation domains of DTPA fragment ions, which was attributed to roughened gold surfaces (36) (**Supplementary Figure 6A**). The roughened surface could be a contributing factor in the characteristic uneven or patchy distribution of organic components during the QCM formulation process.(36-38). This suggested that subsequent imaging of the β -CD and C_{60} would most likely be located within these domains. In fact, **Supporting information Figure 6B** shows some degree of shadowing in the overlayed image (c) since the intensity of Au in (a) appears a little blurred after attachment of the cyclodextrin.

The fully formulated QCM with the chemistry (Au)-S-(CH_2)₂-CONH- β -CD Sensor **4** was analyzed to determine if the intended reaction occurred with the cyclodextrin. The uneven

distribution was again observed in the sample where there was segregation of the acid (DTPA) components to specific spatial domains on the gold substrate (**Supplementary Figure 6A (a)**). Fragment ions associated with cyclodextrin were observed and distributed in the specific domains that were spatially correlated to the domain areas of the acid (DTPA) (**Supplementary Figure 6B(c)**). The distribution of β -CD was more even over the surface versus either of the other components. The reason for this observation could be due to the reduced surface roughness that occurred once the DTPA had been conjugated to the Au surface of the QCM. The large molecular sizes of β -CD, along with the reduction in roughness would make them appear to be covering larger surface areas on the QCM without being restricted to the anchored acid sites. Atomic Force Microscopy (AFM) was used to determine if surface roughness was playing a role in the uneven distribution of the organic components as shown in **Supplementary Figure 7**. The AFM images showed islands of materials spread out over the gold substrate in the same distribution indicated in the ToF-SIMS chemical images. The correlation between the ToF-SIMS and AFM data indicate that despite the uneven surface distribution, there was successful β -CD immobilization chemistry that was not observed in the controls.

Finally, the sensor exposed to control and fullerene solutions were chemically imaged to determine the spatial distribution of the cyclodextrin and C_{60} fragment ions. **Figure 6 a-d** or **e-g** represents initial sensor fabrication steps before exposure to C_{60} (Figure 6 d) or control (Figure 6 h). A keen examination of these figures show there was more shadowing of initial colors for Au, DTPA and β -CD after capturing C_{60} (Figure 6 d) compared to the control (without C_{60}) (Figure 6 h) from the colored overlay images. Additionally, the QCM exposed to the controls had very little signal from the C_{60} fragment ions in comparison with that exposed to fullerene solution. An insignificant ion signal was present in the control but was more likely due to baseline noise in the mass spectra as opposed to C_{60} fragment ions. The fullerene exposed QCM had a distribution of C_{60} fragment ions over the surface of the QCM that was consistent with the domain distribution of the cyclodextrin fragment ions. This confirms not only that the cyclodextrin and C_{60} are present on the surface of the QCM but also that they were spatially distributed in the same domains. Most importantly, this is the first report on successful immobilization of cyclodextrin on QCM surface for the purpose of quantifying engineered fullerene C_{60} particles

Environmental Application: 12 mg of C_{60} and 10 ml of deionized water were added to 1 gram of SRM soil samples and was stirred at 1150 rpm under ambient conditions for 1 hr. 1 ml of anhydrous toluene was added and the resulting mixture was shaken for another 1 hr. C_{60} was extracted into the organic phase. The extraction process was repeated 3 times with 1ml of toluene. The resulting extract was filtered through a 0.20 μ M filter membrane and diluted to make 0.14 mg/ml C_{60} . After capturing C_{60} particles onto the sensor from pure and soil samples, ΔF were 13251 Hz and 9005 Hz, corresponding to 7.42×10^{16} and 5.04×10^{16} particles/cm² respectively (**Figure 5**). In both cases, similar orders of magnitude of the C_{60} particles/cm² were obtained.

Conclusion: We have demonstrated a new analytical concept that can be used to isolate and measure the number of engineered fullerene C_{60} particles from pure and soil samples. Mixtures containing C_{60}/C_{70} were isolated up to 20 fold C_{70} concentration. Utilizing

QCM's mass detection capabilities, we have developed a Category II nanosensor concept based on supramolecular complexation of engineered fullerene nanoparticle onto cyclodextrin. The sensor provides a size-exclusive approach for quantitative analysis of the nominated fullerenes. To the best of our knowledge, this is the first Category II nanosensor reported for monitoring engineered fullerene C₆₀. The structural and morphological validity of the proposed sensor was confirmed using SIMS, NMR and SEM techniques, and the concept should be applicable to other fullerenes based on unique design of the sandwich configuration. We have thus discovered a new practical measurement method for engineered fullerenes C₆₀. Future work will focus on the application of the proposed sensor concept in wastewater samples, consumer products and food supplements.

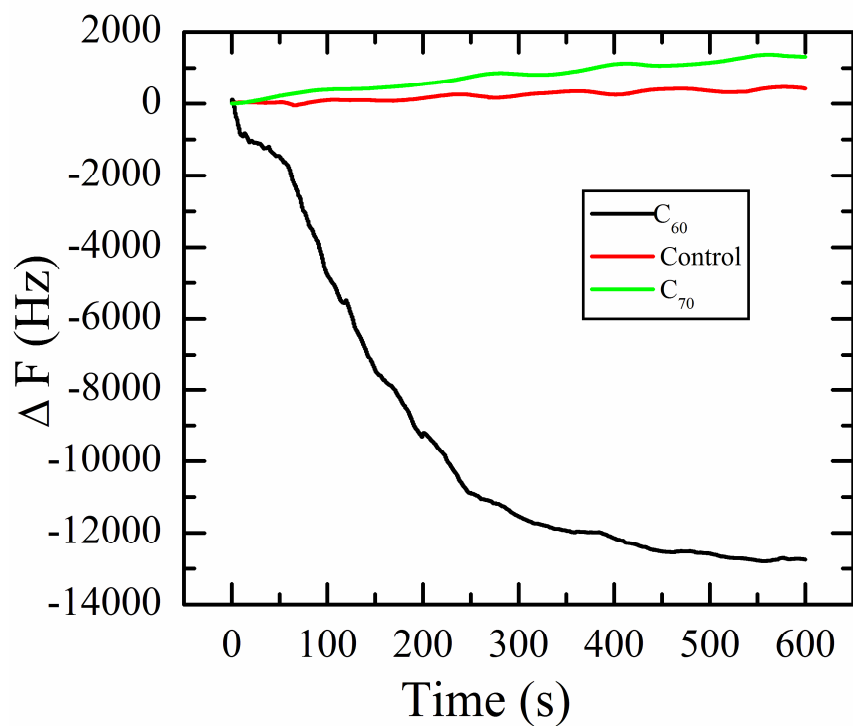


Figure 1: Change in frequency vs time for QCM (Au)-S-(CH₂)₂-CONH-beta-CD sensor, **4** in presence of fullerene 0.14 mg/ml C₆₀, C₇₀ and control (toluene).

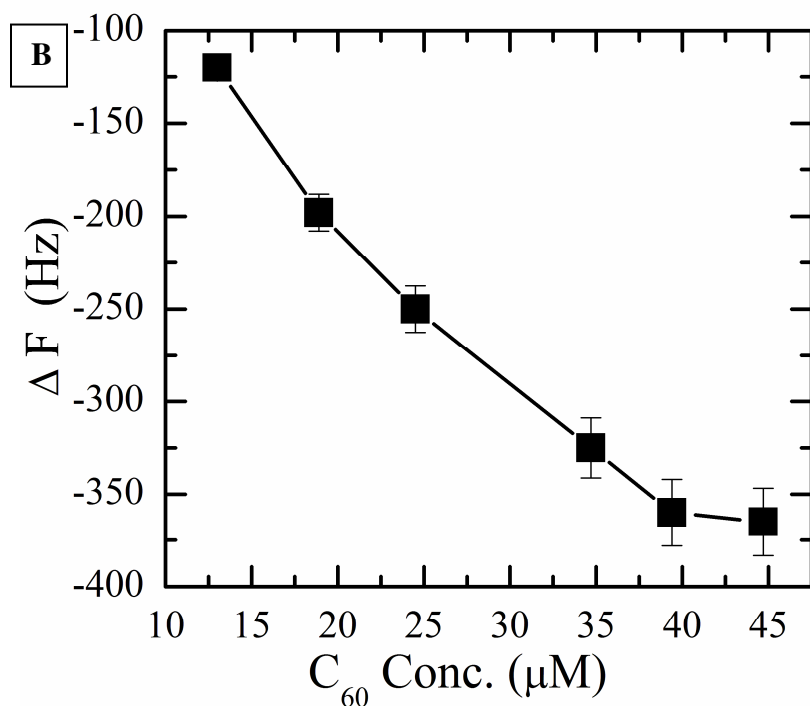
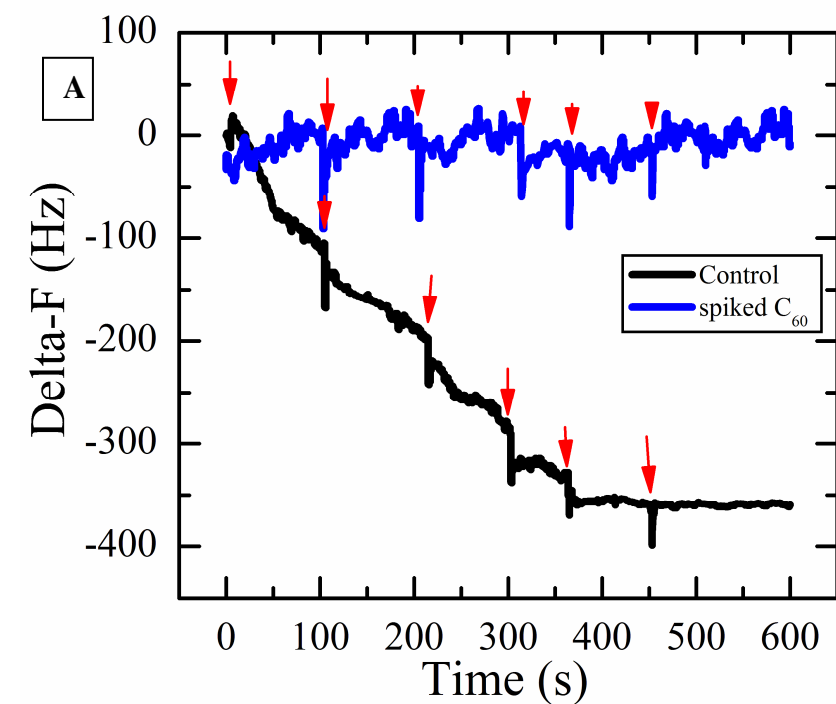


Figure 2: Dose-dependent response of QCM (Au)-S-(CH₂)₂-CONH-beta-CD sensor during the spiking of 200 μ L of (a) Control (toluene only) (b) 0.15 mg C_{60} /ml toluene: Arrows indicate the spiking events (c) Change of frequency versus concentration of spiked C_{60} (μM).

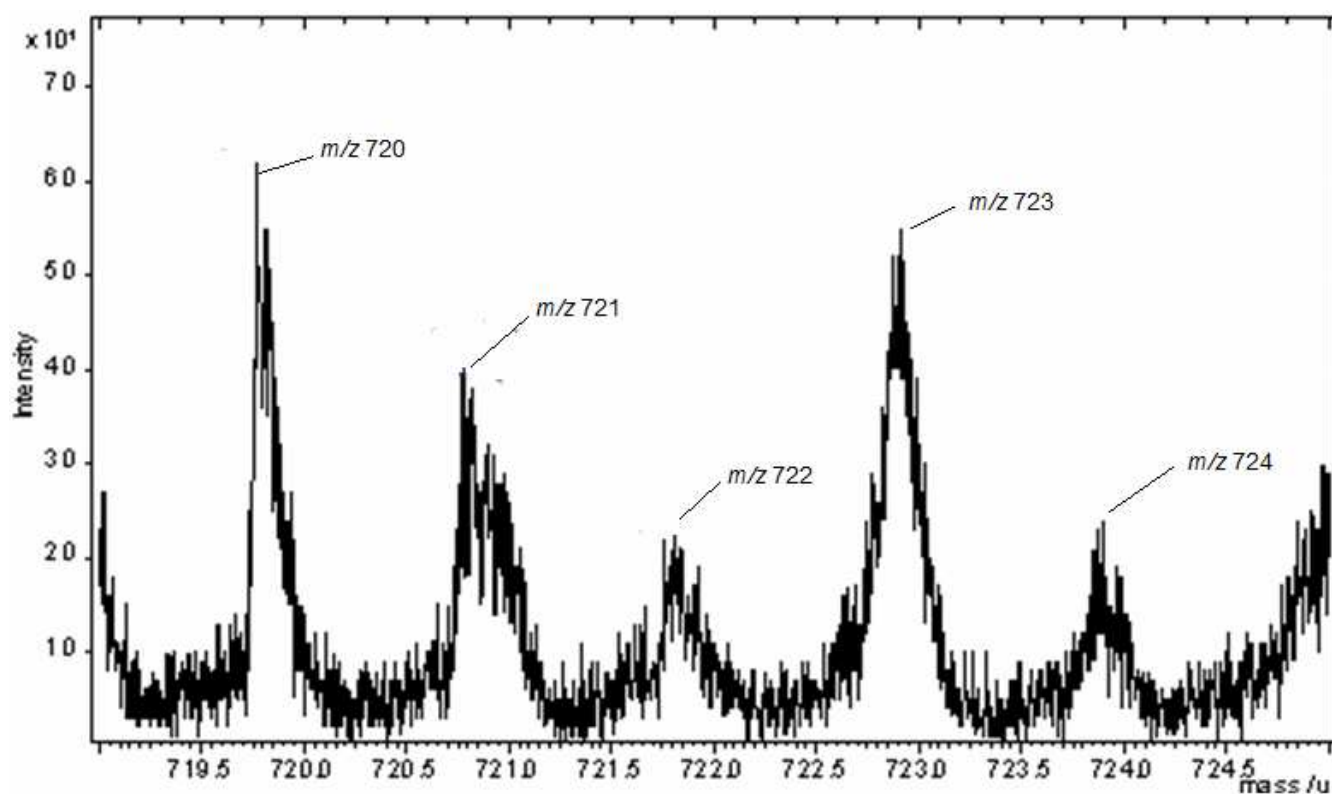


Figure 3: C_{60} mass at m/z 720 and isotopic peaks ($m/z=$ 721, 722, 723 & 724). ToF-SIMS mass spectrum was acquired in the negative ion acquisition mode.

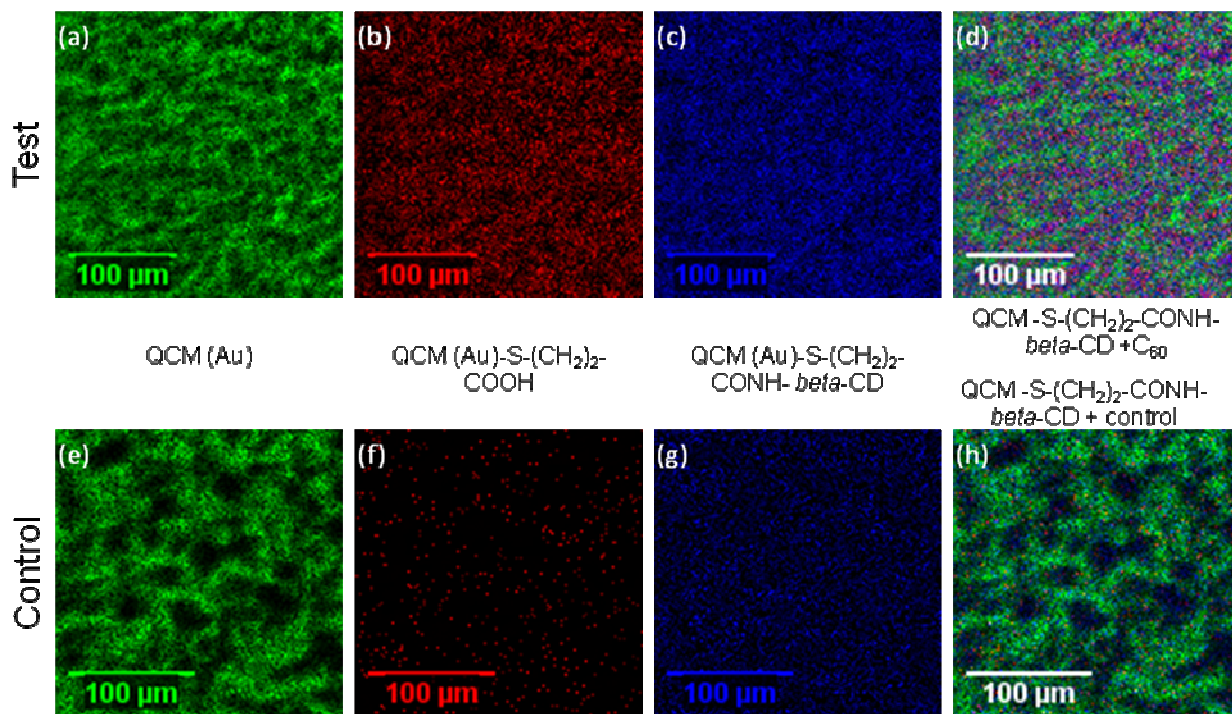


Figure 4: False color ToF-SIMS chemical image of QCM (Au)-S-(CH₂)₂-CONH-β-CD showing same stepwise sensor fabrication components (a-c and e-g) and overly of the three colored images after exposure to fullerene C₆₀ (d) and control (h). Colored overlay image prepared using Ion Image® Software Package, scale bar added using Image J (35).

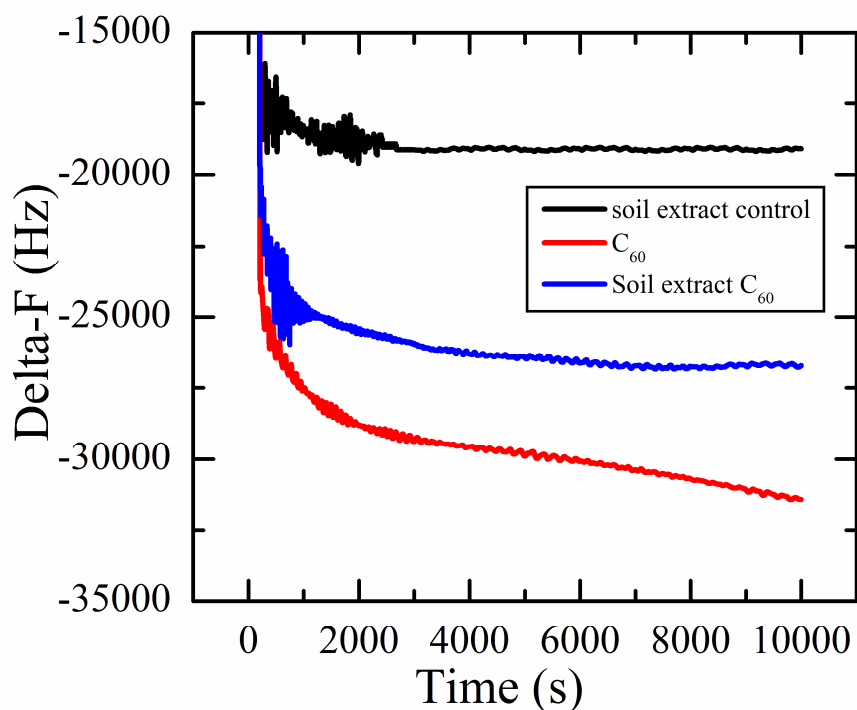


Figure 5: Change in frequency vs time for QCM (Au)-S-(CH₂)₂-CONH-beta-CD sensor, **4** in presence of fullerene 0.14 mg/ml C₆₀, C₆₀ soil extract and control (toluene soil extract).

Supporting Information. Additional information on sensor synthesis, chemistry, characterization using ToF-SIMS and response to C₇₀ and C₇₀/C₆₀ mixture. (Figure S1-7; Tables S1, S2; Scheme 1). This information is available free of charge via the Internet at <http://pubs.acs.org>.


Notice: The United States Environmental Protection Agency through its Office of Research and Development (funded and collaborated in) the research described here under Student Services Contract #RFQ-RT-08-00130 to Samuel Kikandi and the STAR Program #RD-83409101 to Omowunmi Sadik at SUNY-Binghamton. It has been subjected to Agency review and approved for publication.

Literature cited

- (1) Sadik.O.A.; S., K.; Wang.C.Q.; K.Varner., Sensors as tools for quantitation, nanotoxicity and nanomonitoring assessment of engineered nanomaterials. *Journal of environmental monitoring* **2009**, *11*, 1782-1800.
- (2) <http://www.epa.gov/osa/pdfs/nanotech/epa-nanotechnology-whitepaper-0207.pdf>
- (3) Yamawaki, H.; Iwai, N., Cytotoxicity of water-soluble fullerene in vascular endothelial cells. *American Journal of Physiology-Cell Physiology* **2006**, *290*, (6), C1495-C1502.
- (4) Yang, X. L.; Fan, C. H.; Zhu, H. S., Photo-induced cytotoxicity of malonic acid [C60]fullerene derivatives and its mechanism. *Toxicology in Vitro* **2002**, *16*, (1), 41-46.
- (5) Isaacson, C. W.; Kleber, M.; Field, J. A., Quantitative Analysis of Fullerene Nanomaterials in Environmental Systems: A Critical Review. *Environmental Science & Technology* **2009**, *43*, (17), 6463-6474.
- (6) Sayes, C. M.; Fortner, J. D.; Guo, W.; Lyon, D.; Boyd, A. M.; Ausman, K. D.; Tao, Y. J.; Sitharaman, B.; Wilson, L. J.; Hughes, J. B.; West, J. L.; Colvin, V. L., The Differential Cytotoxicity of Water-Soluble Fullerenes. *Nano Letters* **2004**, *4*, (10), 1881-1887.

- (7) Isakovic, A.; Markovic, Z.; Todorovic-Markovic, B.; Nikolic, N.; Vranjes-Djuric, S.; Mirkovic, M.; Dramicanin, M.; Harhaji, L.; Raicevic, N.; Nikolic, Z.; Trajkovic, V., Distinct cytotoxic mechanisms of pristine versus hydroxylated fullerene. *Toxicological Sciences* **2006**, *91*, (1), 173-183.
- (8) Zakharenko, L. P.; Zakharov, I. K.; Vasyunina, E. A.; Karamysheva, T. V.; Danilenko, A. M.; Nikiforov, A. A., Determination of genotoxicity of fullerene C-60 and fullerol by the somatic mutation and recombination test in *Drosophila melanogaster* and SOS chromotest. *Genetika* **1997**, *33*, (3), 405-409.
- (9) Sadik, O. A., Detecting engineered nanomaterials. *Journal of Environmental Monitoring* **2007**, *9*, (11), 1154-1154.
- (10) S. Andreescu; J. Njagi; C. Ispas; Ravalli, M. T., JEM Spotlight: Applications of advanced nanomaterials for environmental monitoring. *J. Environ. Monit.*, **2009**, *11*, 27-40.
- (11) Wei, D.; Bailey, M. J. A.; Andrew, P.; Ryhanen, T., Electrochemical biosensors at the nanoscale. *Lab on a Chip* **2009**, *9*, (15), 2123-2131.
- (12) Murthy, C. N.; Geckeler, K. E., The water-soluble beta-cyclodextrin-[60]fullerene complex. *Chemical Communications* **2001**, (13), 1194-1195.
- (13) Giacalone, F.; D'Anna, F.; Giacalone, R.; Gruttadauria, M.; Riela, S.; Noto, R., Cyclodextrin-[60]fullerene conjugates: synthesis, characterization, and electrochemical behavior. *Tetrahedron Letters* **2006**, *47*, (46), 8105-8108.
- (14) T. Anderson, K. N., M. Sundahl, G. Westman and O. Wennerström., *J. Chem. Soc., Chem. Commun.* **1992**, 604-606.
- (15) Aluoch, A. O.; Sadik, O. A.; Bedi, G., Development of an oral biosensor for salivary amylase using a monodispersed silver for signal amplification. *Analytical Biochemistry* **2005**, *340* 136-144.
- (16) Liu, Y.; Yang, Y. W.; Chen, Y., Thio[2-(benzoylamino)ethylamino-beta-CD fragment modified gold nanoparticles as recycling extractors for [60]fullerene. *Chemical Communications* **2005**, (33), 4208-4210.
- (17) Nishijo, J.; Moriyama, S.; Shiota, S., Interactions of cholesterol with cyclodextrins in aqueous solution. *Chemical & Pharmaceutical Bulletin* **2003**, *51*, (11), 1253-1257.
- (18) Murthy, C. N.; Geckeler, K. E., Stability studies on the water-soluble beta-cyclodextrin [60]fullerene inclusion complex. *Fullerenes Nanotubes and Carbon Nanostructures* **2002**, *10*, (2), 91-98.
- (19) Wrobel, N.; Schinkinger, M.; Mirsky, V. M., A novel ultraviolet assay for testing side reactions of carbodiimides. *Analytical Biochemistry* **2002**, *305*, (2), 135-138.
- (20) Taylor, R., *Lecture Notes on Fullerene Chemistry: A Handbook for Chemists*. Imperial College Press: London, UK., 1999.
- (21) Jinno, K., *Separation of Fullerenes by Liquid Chromatography*. The Royal Society of Chemistry: Cambridge, UK, 1999.
- (22) Haino, T.; Yanase, M.; Fukunaga, C.; Fukazawa, Y., Fullerene encapsulation with calix[5]arenes. *Tetrahedron* **2006**, *62*, (9), 2025-2035.
- (23) Michal Lahav; Koodali T. Ranjit; Eugenii Katz; Willner, I., A b-amino-cyclodextrin monolayer-modified Au electrode: a command surface for the amperometric and microgravimetric transduction of optical signals recorded by a photoisomerizable bipyridinium-azobenzene diad. *Chem. Commun.* **1997**, 259.
- (24) Saurbrey, G. Z., *Z. Phys* **1959**, *155*, 206
- (25) Stobiecka, M.; Ciesla, J. M.; Janowska, B.; Tudek, B.; Radecka, H., Piezoelectric sensor for determination of genetically modified soybean roundup ready((R)) in samples not amplified by PCR. *Sensors* **2007**, *7*, (8), 1462-1479.
- (26) Bulavin, L. A.; Adamenko, I. I.; Yashchuk, V. M.; Ogul'chansky, T. Y.; Prylutsky, Y. I.; Durov, S. S.; Scharff, P., Self-organization C60 nanoparticles in toluene solution. *Journal of Molecular Liquids* **2001**, *93*, (1-3), 187-191.
- (27) Lee, J. Y.; Park, S. M., Electrochemistry of guest molecules in thiolated cyclodextrin self-assembled monolayers: An implication for size-selective sensors. *Journal of Physical Chemistry B* **1998**, *102*, (49), 9940-9945.
- (28) Aluoch, A. O.; Amrute, K.; Sadik, O. A., Novel electrochemical oral biosensor for histatin. *Sensor Letters* **2005**, *3*, (2), 161-163.
- (29) Kollmer, F., Cluster primary ion bombardment of organic materials. *Applied Surface Science* **2004**, *231-232*, 153-158.
- (30) Rabara, L.; Aranyosiova, M.; Velic, D., Supramolecular host-guest complexes based on cyclodextrin-diphenylhexatriene. *Applied Surface Science* **2006**, *525*, 7000-7002.
- (31) O'Brien, S. C.; Heath, J. R.; Curl, R. F.; Smalley, R. E., Photophysics of buckminsterfullerene and other carbon cluster ions. *Journal of Chemical Physics* **1988**, *88*, (1), 220-232.
- (32) Kato, N.; Yamashita, Y.; Iida, S.; Sanada, N.; Kudo, M., Analysis of ToF-SIMS spectra from fullerene compounds. *Applied Surface Science* **2008**, *225*, 938-940.
- (33) <http://www.zeiss.com/c1256e4600305472/Contents-Frame/c4bc1c66687fdce1c1256fe100420194>
- (34) Rudalevige, T.; Francis, A. H.; Zand, R., Spectroscopic studies of fullerene aggregates. *Journal of Physical Chemistry A* **1998**, *102*, (48), 9797-9802.
- (35) Collins, T. J., ImageJ for microscopy. *BioTechniques* **2007**, *43*, S25-S30.

- (36) Reimhult, K.; Yoshimatsu, K.; Risveden, K.; Chen, S.; Ye, L.; Rozer, A., Characterization of QCM sensor surfaces coated with molecularly imprinted nanoparticles. *Biosensors and Bioelectronics* 2008 **2008**, 23, 1908-1914.
- (37) Briand, E.; Gu, C.; Boujday, S.; Salmain, M.; Herry, J. M.; Pradier, C. M., Functionalisation of gold surfaces with thiolate SAMs: Topography/bioactivity relationship – A combined FT-RAIRS, AFM and QCM investigation. . *Surface Science* **2007**, 601, 3850-3855.
- (38) Parra, A.; Casero, E.; Pariente, F.; Vazquez, L.; Lorenzo, E., Bioanalytical device based on cholesterol oxidase-bonded SAM-modified electrodes. *Analytical and Bioanalytical Chemistry* **2007**, 388 1059-1067.

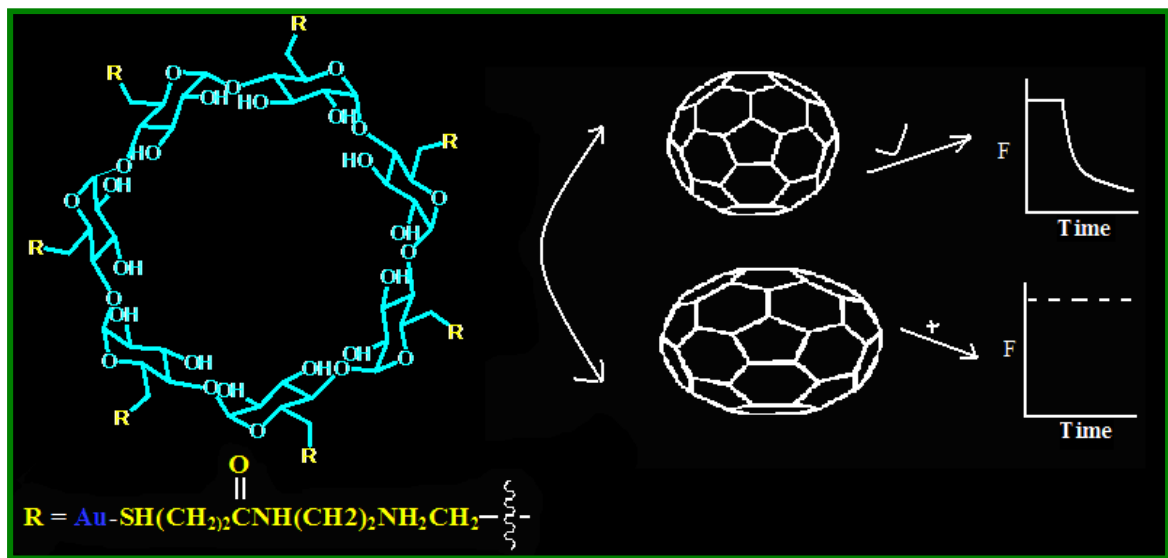

Size-exclusive nanosensor for quantitative analysis of fullerene