




EPA/ORD Method for SARS-CoV-2 Wastewater Monitoring

Nichole Brinkman


US Environmental Protection Agency
Office of Research and Development



The views expressed in this presentation are those of the author(s) and do not necessarily represent the views or policies of the U.S. Environmental Protection Agency. Any mention of trade names or commercial products does not constitute EPA endorsement or recommendation for use.



OH Coronavirus Wastewater Monitoring Network

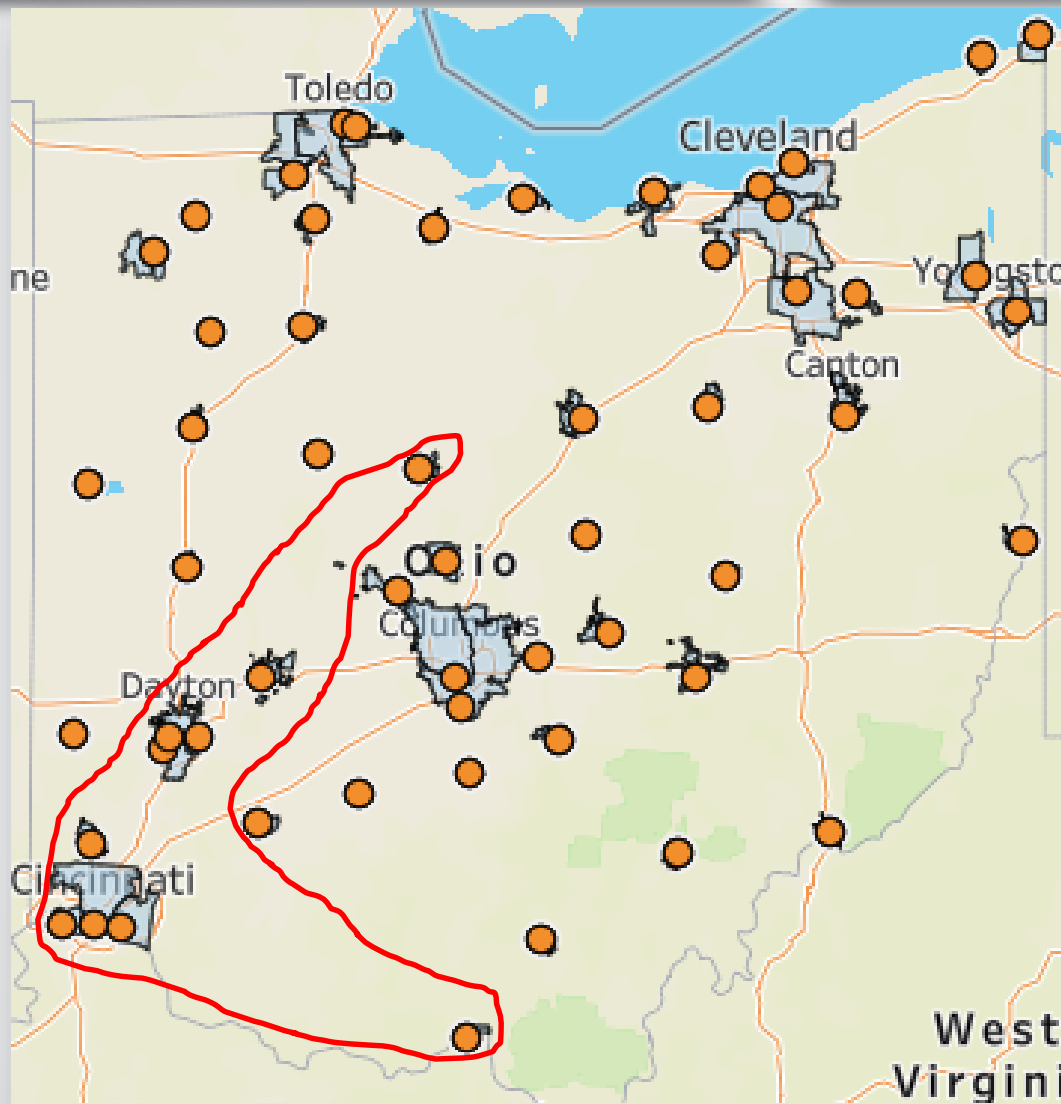

- Initiated in May by Gov. DeWine
- Coordinated by Ohio Water Resources Center at OSU
 - Ohio Department of Health
 - Ohio EPA
 - 56 wastewater utilities
 - University labs
 - Commercial labs
 - USEPA/ORD-Cincinnati





Mill Creek Sewershed

Sewershed boundary



Coming soon: Daily new case counts in sewershed

Viral Gene Copy Trends





Method Considerations

Sample Type


Untreated wastewater
Primary sludge
Volume

Sample Preparation

Storage temperature
Homogenization
Additives
Matrix Spike
Clarification

Sample Concentration

Ultrafiltration

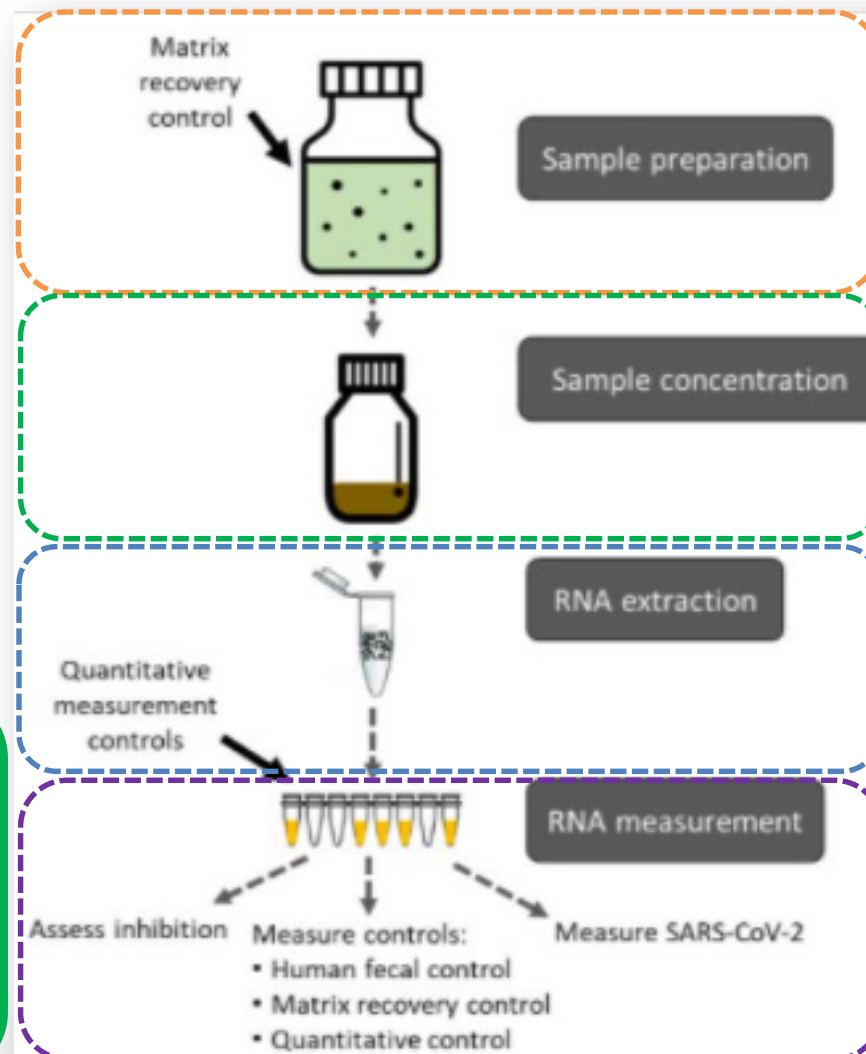

Nucleic Acid Extraction

Silica columns
Magnetic beads
Precipitation

RNA/DNA Measurement


RT-qPCR
RT-ddPCR
Genetic targets

Other Considerations

Biosafety
Supply Chain issues
Practicality (time, equipment)
QA/QC



Sample Processing and Analysis

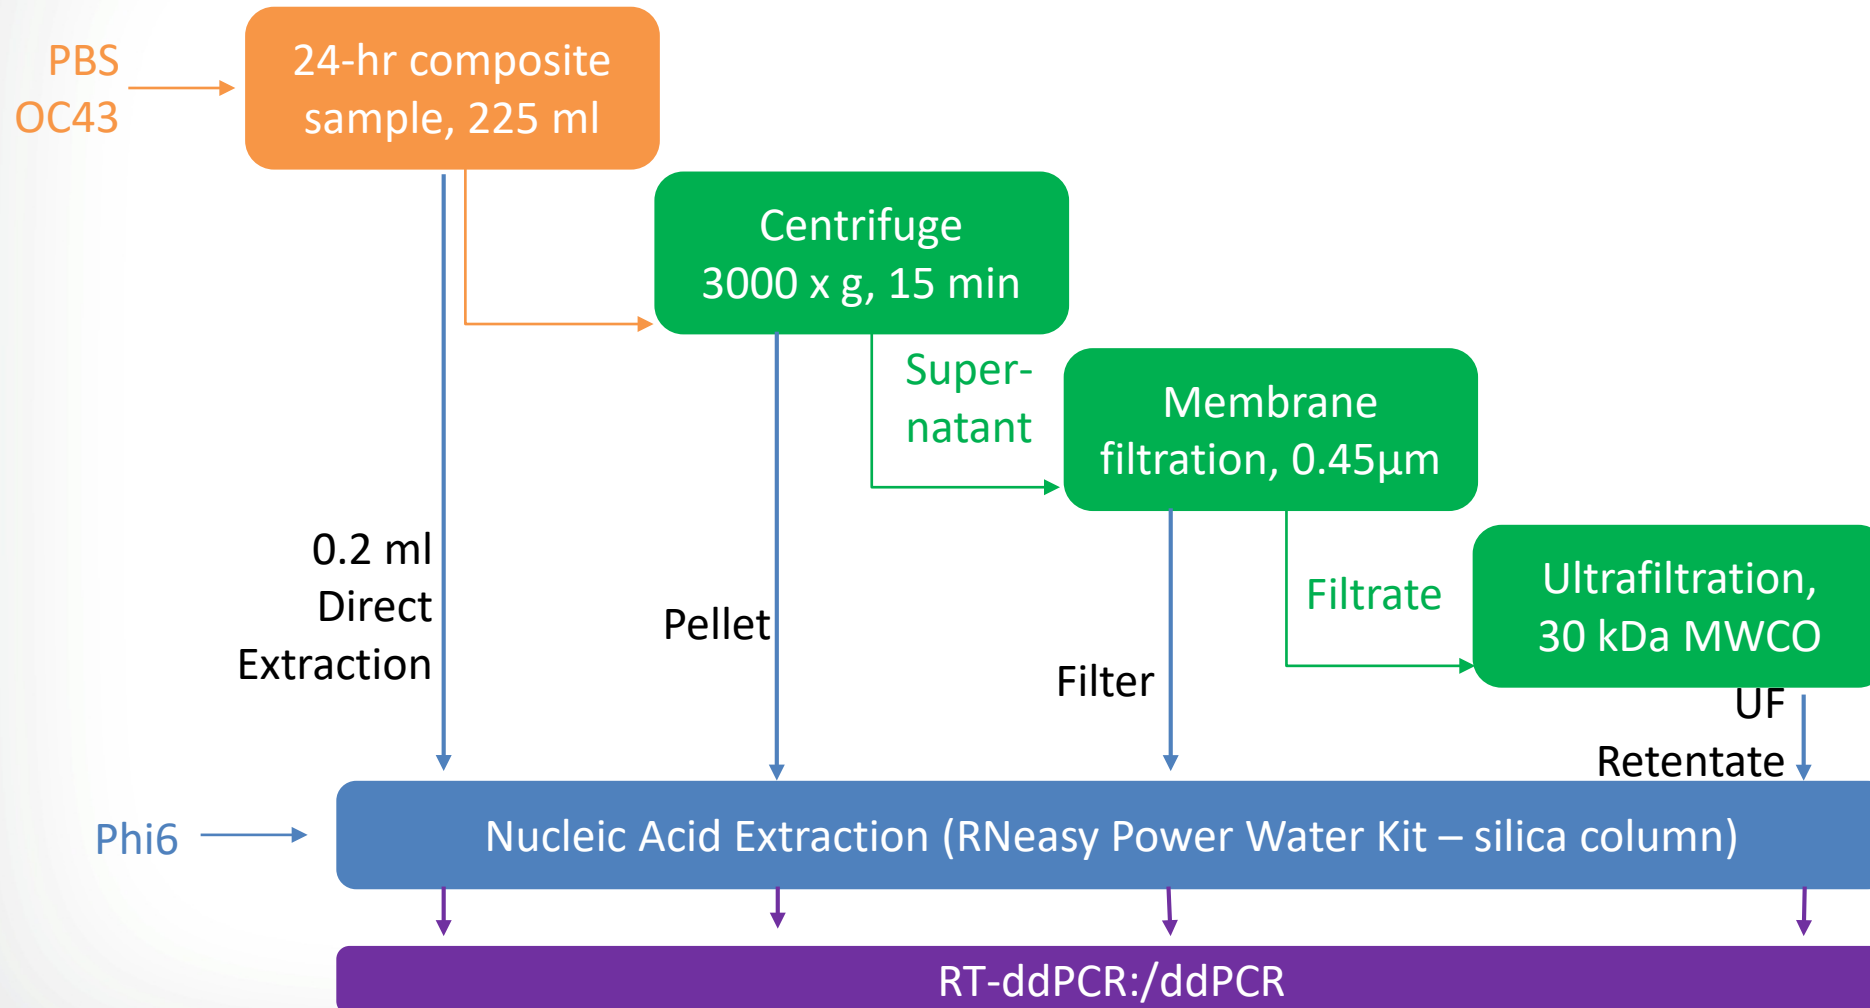


SARS-CoV-2 (N1, N2), RT-ddPCR QC, Inhibition control, Extraction Control, Matrix Recovery Control, Human fecal marker



Limits of Detection/Quantification


- **Volume of sample processed**
- **Concentration factor**
- **Volume of processed sample analyzed**
- **Analytical sensitivity (i.e., minimum detectable concentration)**
- **Ideal conditions**
- **Practical limits likely higher due to losses during processing**





Recovery Efficiency of Endogenous and Spiked Virus


- **Endogenous virus**
 - crAssphage
 - Pepper Mild Mottle Virus
- **Spiked virus**
 - OC43
- **Measure concentrations before and after sample processing**





Partitioning of Virus in Sample Fractions


- **Where are viruses recovered within samples?**
- **Proportion of total virus measured in each sample fraction**
- **~ 90% measurable virus in pellet and filter fractions**

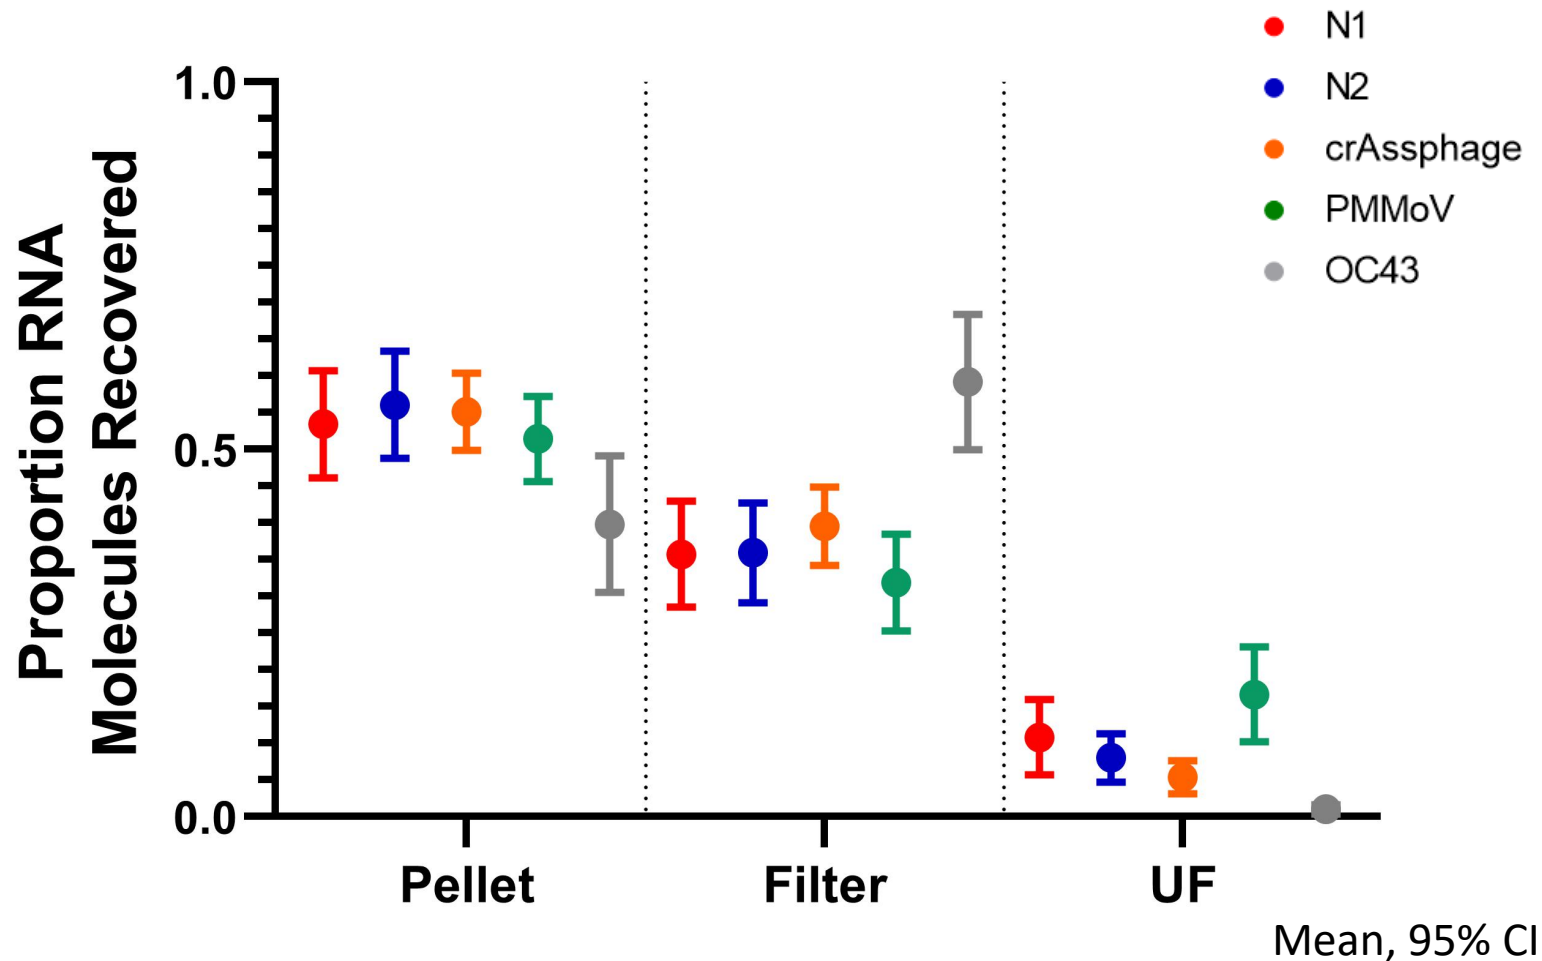




RT-ddPCR Inhibition

- **Add RNA before RT-ddPCR**
- **Compare RNA concentration in sewage sample extracts and matrix-free controls**
- **Minimal RT-ddPCR inhibition observed**







Supply Chain Issues

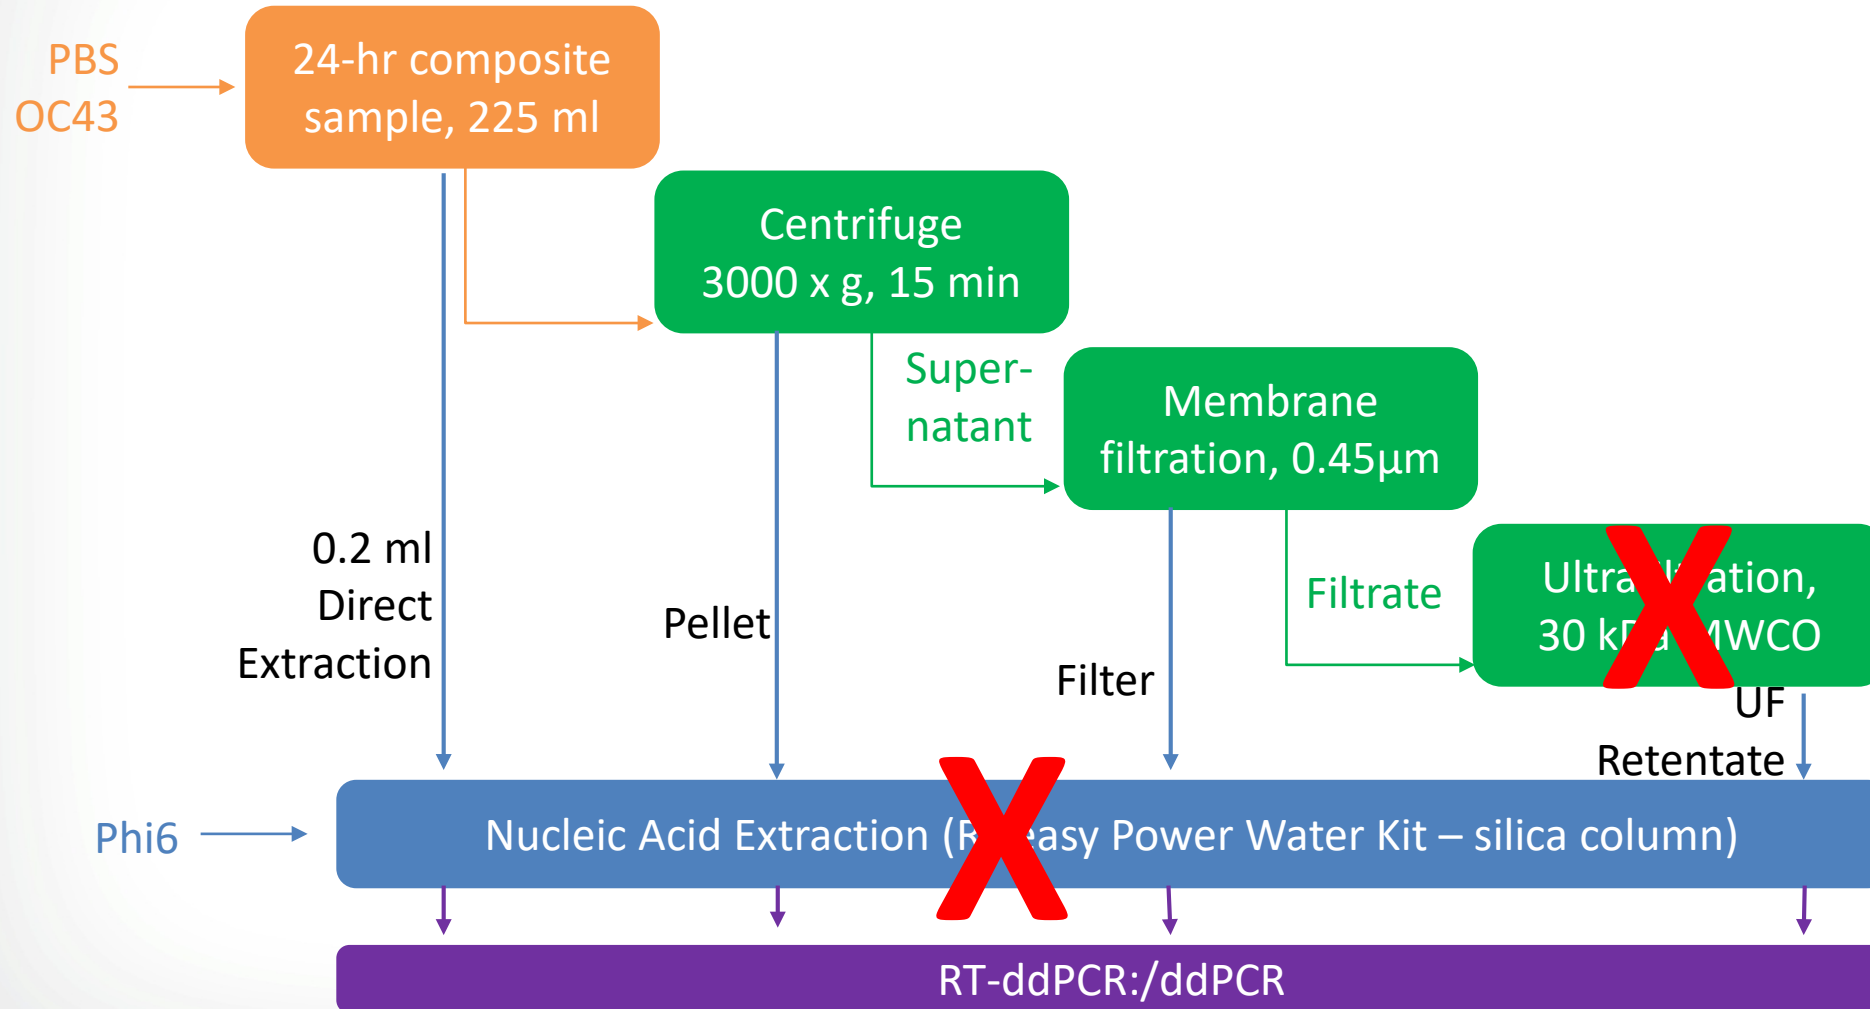


SARS-CoV-2 (N1, N2), RT-ddPCR QC, Inhibition control, Extraction Control, Matrix Recovery Control, Human fecal marker

SARS-CoV-2 N1, N2 concentrations




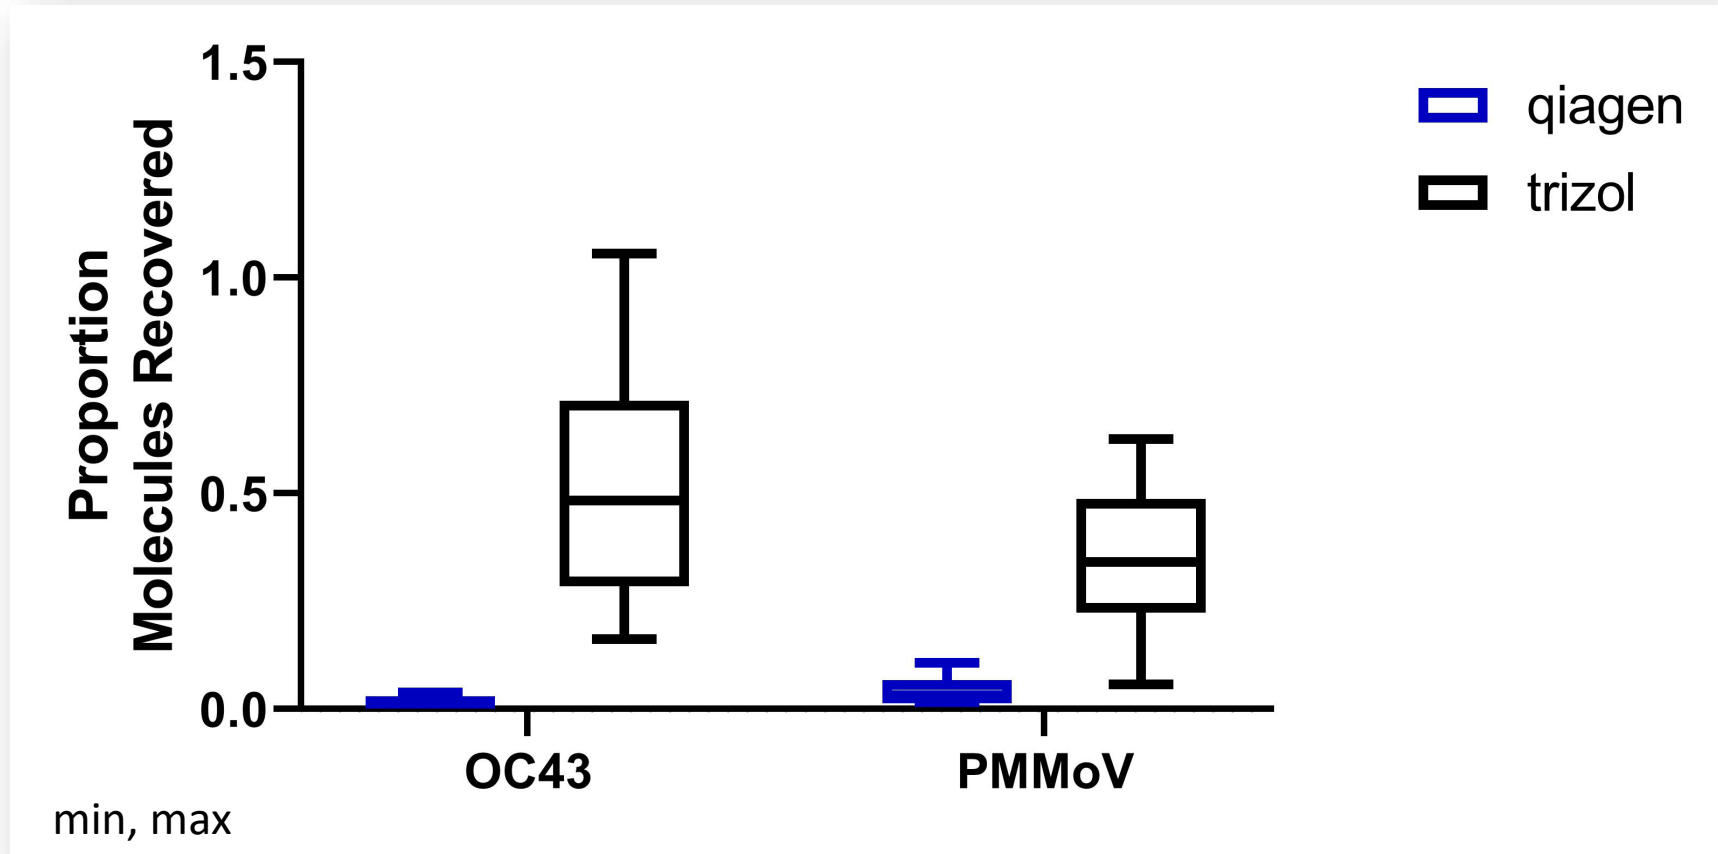



Sample Storage at 4°C

- 24- hour composite
- Shipped overnight
- How long can samples be stored before a significant decrease in viral RNA is observed?
- No significant difference in SARS-CoV-2 RNA up to 4 days at 4°C





p-values for repeated measures ANOVA with time



Sample Storage at -70°C


- What is the effect of freeze-thaw cycle on detection of SARS-CoV-2 RNA?
- Sample collected and processed immediately
- Subsample frozen at -70°C, thawed at 37°C






Temporal Trends of SARS-CoV-2 in Sewersheds


Mill Creek




Muddy Creek




Taylor Creek




Little Miami




Dayton




Western Regional




Eastern Regional




Springfield




Marion



Portsmouth



Hamilton



- **Wastewater is a complex and variable matrix**
- **No standard method for measuring SARS-CoV-2, but many options available**
- **Quality Control important for assessing method performance and matrix variability**
- **Supply chain can be disrupted**
- **Sample handling conditions – need more data**
 - **Temporary storage – no reduction at 4°C up to 4 days**
 - **Long-term storage – up to 5-fold reduction after freezing at -80 °C**
- **Continue to measure SARS-CoV-2 in wastewater at specified sites**
- **Focus on trends or significant changes in the concentration of viral RNA detected**
- **Continue to work with ODH to interpret trends for appropriate public health applications**



Research Team and Partners

EPA/ORD

Emily Wheaton
Maitreyi Nagarkar
Chloe Hart
Scott Keely
Michael Jahne
Alison Franklin
Eunice Varughese
Jay Garland
Laura Boczek
Randy Revetta
Brian Morris
Dave Feldhake
Ana Braam
Barry Wiechman
Sarah Okrum
Jacob Botkins
Leah Julifs

Utilities

Metropolitan Sewer District of Greater Cincinnati

Bruce Smith

City of Dayton

Chris Clark, Walter Schroder

City of Marion

Steve Morris

City of Portsmouth

Tommy Stewart

Montgomery County

Jim Davis

City of Hamilton

Mark Smith

City of Springfield

Jeff Yinger

Hamilton County Public Health Department

Chris Griffith

Ohio Water Resources Center

Zuzana Bohrerova

Ohio Department of Health

Rebecca Fugitt

Ohio EPA

Brian Hall

Tiffani Kavalec

University Labs

Ohio State University

University of Toledo

Kent State University

University of Akron